## Why Do Scientists Choose the DS-11 Series?

Nano UV-Vis, Fluorescence and Cuvette Unmatched Specificity and Sensitivity

Powerful EasyApps™ Software
Designed by Life Scientists, for Life Scientists

Multi-Award Winning
The World's Top Rated Spectrophotometer

Flexible Export and Connectivity Wi-Fi, USB, Email, Ethernet and more

# Rapid and Reliable 1 µL UV-Vis






## SmartPath™ Technology

The DeNovix team developed a combination of opto-mechanical components and software algorithms that optimize results for every sample. Micron-level pathlength control and immediate absorbance feedback deliver the most sensitive and accurate microvolume measurements.

**Bridge Testing™** verification eliminates unreliable results that stem from broken sample columns or loading issues. The algorithm detects unbridged samples and automatically adjusts in real-time to deliver accurate results, even for challenging 1 µL protein samples.

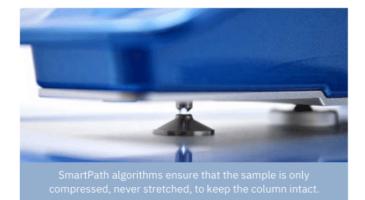

## **Key Features**

- · Quantify DNA, RNA and protein in less than 3 sec
- Widest dynamic range and lowest detection limit 0.75 37500 ng/µL dsDNA
- · No routine maintenance or recalibration required
- $\bullet$  Full spectrum UV-Vis analysis using 0.5 1.0  $\mu L$  of sample

## SmartQC™ Contamination Alerts

Multiple algorithms ensure confidence in results while also providing important information about possible sample anomalies.

Surface Check	Smar tPath™	Bridge Testing™	Spectral Analysis	Aler t	Repor t
Check that previous sample has been removed.	Precisely select optimum pathlength for each sample.	Dynamic monitoring and adjustment ensures that sample column is formed.	Analyze for negative spectra, absorbance, within range, calculate purity ratios and quantify.	Check against threshold purity values. Flag contaminated samples. Display user guidance.	Save and report data ready for export. Optional auto-save to network drive.

## Choice of Modes for Total Sample QC

Combine the ease of use, wide dynamic range and contamination detection of UV-Vis with the enhanced sensitivity and specificity of fluorescence quantification. Achieve total sample quality control and unmatched flexibility for current and future assay compatibility.

MODELS			
DS-11 FX+	<b>✓</b>	<b>✓</b>	<b>✓</b>
DS-11 FX	<b>✓</b>	<b>✓</b>	
DS-11 +	<b>✓</b>		<b>✓</b>
DS-11	<b>✓</b>		

## **Integrated Fluorescence**



The DS-11 Series uniquely integrates an optional 4-channel fluorometer. Fluorescence mode enables up to 1000x more sensitivity. DeNovix Fluorometers are compatible with a wide range of commonly used quantification assays.



Extend the lower detection limit for low concentration samples. Quantify down to 0.5 pg/  $\mu L$  dsDNA.




Selectively quantify a sample in the presence of contaminants using DeNovix Fluorescence Quantification Assays.



Combine Absorbance and Fluorescence measurements for specific quantification and reliable contamination detection.



#### DeNovix Fluorometers and Assays Combine for Unmatched Sensitivity

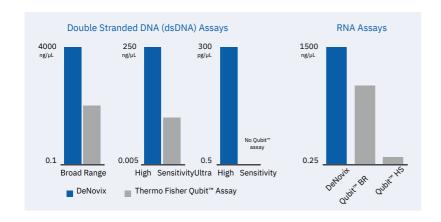

#### **Key Features**

- Full range of dsDNA and RNA assay kits
- Simple mix-and-measure, 2-point standard protocol
- Outperforms equivalent Thermo Fisher Qubit™
   assay kits in both sensitivity and dynamic range

## **Cuvette Absorbance**



Use standard quartz or disposable cuvettes for up to 10 mm pathlength absorbance measurements (190 – 840 nm).

Cuvette applications include nucleic acids, proteins, colorimetric assays, OD600 and custom standard curves. Systems include a cuvette block heater for Kinetics studies from 37 – 45°C.



### **Extended Product Line**



#### **QFX Fluorometer**

Affordable, ultra-sensitive 4-channel fluorometer with software pre-installed for commercially popular assays. Includes full network connectivity.



## **DS-C Spectrophotometer**

Cuvette-only instrument for UV-Vis applications (190 - 840 nm). Intuitive operation, full connectivity and pre-installed network EasyApps for rapid quantification.



#### FX Fluorometer Module

Add the USB connected FX Module to any DS-11 Series Spectrophotometer to enable all DeNovix Fluorometer apps. Features the same sensitivity and 4-channel flexibility as the DS-11 FX+, DS-11 FX and QFX.

#### **Spectrophotometer Microvolume Mode** (DS-11, DS-11+, DS-11 FX, DS-11 FX+)

Minimum Sample Size  $0.5~\mu L$ 

Pathlength 0.5 mm (auto ranging to 0.020 mm)

Light Source Pulsed Xenon flash lamp

Detector Type 2048 element CCD

Wavelength Range 190 - 840 nm Wavelength Accuracy 0.5 nm

Absorbance Precision 0.015 AU (1 cm) or 1%, whichever is greater

Absorbance Accuracy 1.5% at 0.75 AU at 260 nm

Spectral Resolution 1.50 FWHM @253.65 nm

**Absorbance Range** 0.015 – 750A (1 cm)

Detection Limit 0.04 mg/mL BSA; 0.75 ng/μL dsDNA Maximum

Concentration 1125 mg/mL BSA; 37500 ng/ $\mu$ L dsDNA Measurement Time 2 seconds

**AutoRun Function** Yes

Power Consumption 10 W (max 30 W)

**Contaminant Detection** SmartQC<sup>™</sup> contamination alerts

#### Spectrophotometer Cuvette Mode (DS-11+, DS-11 FX+, DS-C)

Beam height 8.5 mm

Heating 37 - 45°C +/- 0.5°C

**Pathlength** 10, 5, 2, 1, 0.5, 0.2, 0.125 mm

Detection Limit 0.002 mg/mL BSA (1 cm)

0.04 ng/µL dsDNA (1 cm)

Maximum Concentration 75.0 ng/µL dsDNA (1 cm)

#### Fluorometer Mode (DS-11 FX, DS-11 FX+, QFX, FX Module)

LED Sources UV (375 nm), Blue (470 nm),

Green (525 nm), Red (635 nm)

**Excitation Filters** UV (361-389 nm), Blue (442-497 nm),

Green (490-558 nm), Red (613-662 nm)

Emission Filters 435-485 nm, 514-567 nm,

565-650 nm, 665-740 nm

Detectors Photodiode, detection range 300-1000 nm Tube Type 0.5 mL

thin-wall PCR tubes

Display 7" high definition color display

Touch Screen Projective capacitive

Gesture Recognition Multipoint touch, swipe, pinch

Glove Compatibility All common lab gloves

Internal Storage 32 GB flash memory

Connectivity Wi-Fi, Ethernet, 3 USB ports

Accessories Printer; barcode reader, keyboard, mouse

Weight 2 kg

Footprint 20 cm X 33 cm

Operating Voltage 12 VDC

Approvals UL/CSA, CE, FCC, Japan CAB

**Manufacture Location** USA

Warranty 2 Year Standard

Colors (DS-11 Series)

Patented Design US9442009. Apparatus and Method for Making Optical Measurements of Samples

Copyright ©2022 DeNovix Inc. 24-MAR-2022

Oubit™ is a registered trademark of Thermo Fisher Scientific



Email: info@denovix.con